


# HPLC System Trouble Shooting

Common causes for abnormal chromatograms

## Unstable baseline values

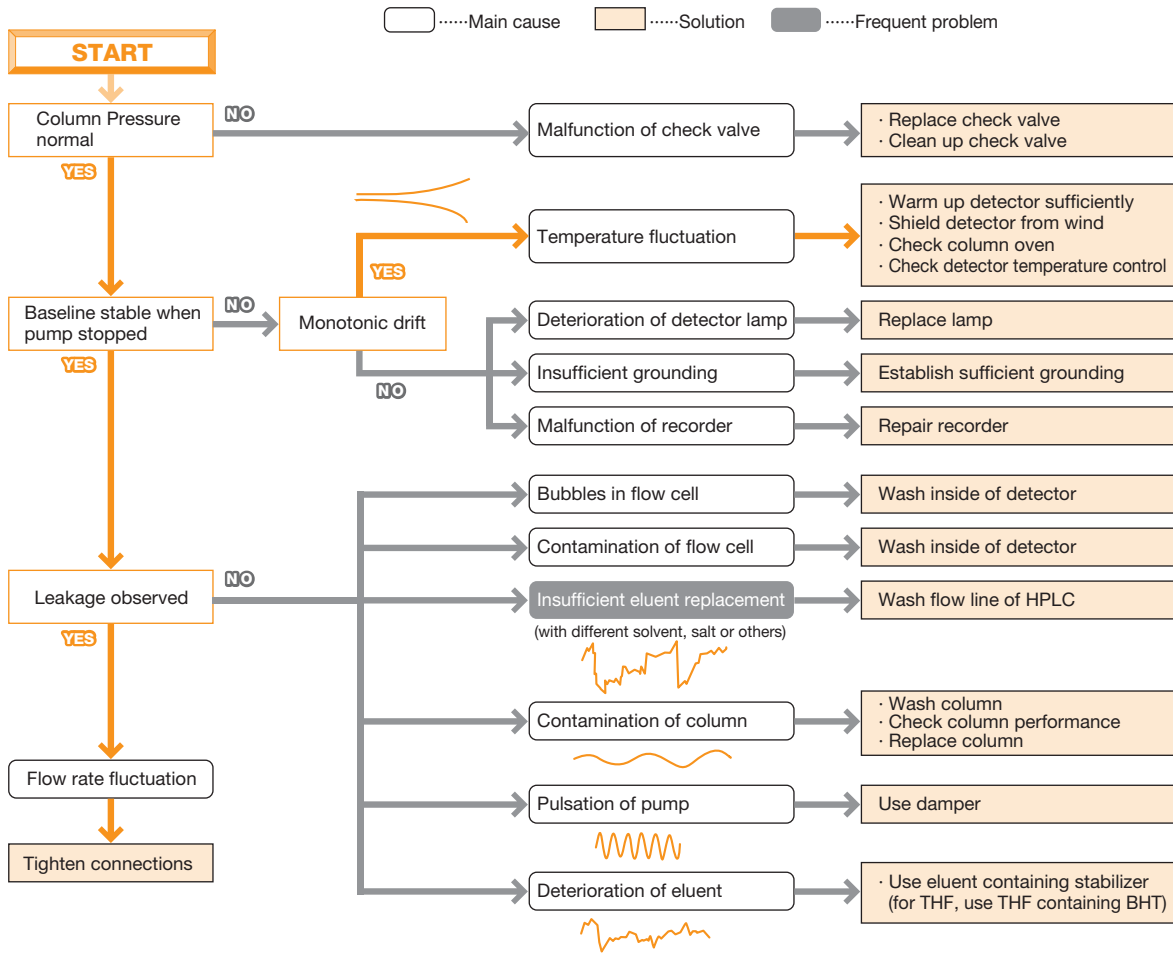

## Noise

